


QUICK REFERENCE SHEET

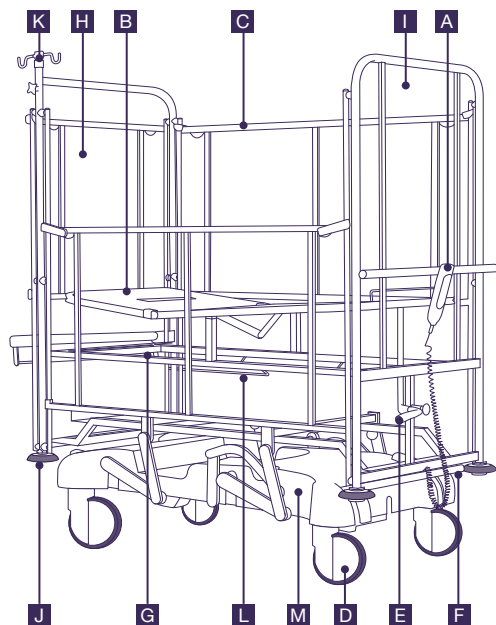

CRIB'S COMPONENTS

A	Control with cable	H	Headboard
B	Crib base	I	Footboard
C	Adjustable side rails	J	Bumpers
D	Wheels	K	IV Pole
E	Trendelenburg / Antitrendelenburg lever	L	Multi-support
F	Braking pedal	M	Fairing
G	Removable tray		

OTHER FUNCTIONS

Trendelenburg / Reverse Trendelenburg mechanism:


This manually **positioning device** allows the crib to be positioned in Trendelenburg and Reverse trendelenburg position.

Raising / lowering the side rails (2):


- To raise them, pull them upwards.
- To lower them, unlock the triggers and follow the side rails as they are lowered.

Braking pedal (3):


- Free movement: pedal in the middle position.
- Steering wheel: pedal en its highest position.
- Brake: Pedal en its lowest position.




1.1. Trendelenburg / Reverse trendelenburg lever position




1.2. Trendelenburg position




1.3. Reverse Trendelenburg position




2.1. Unlocking and lowering the triggers




2.2. Correct way to descend triggers




2.3. Accompanyng side rails



3.1. Free movement



3.2. Steering wheel



3.3. Brake

CLEANING

Daily cleaning and disinfection with up to a 1000 ppm concentration of chlorine solutions:

- Headboard, footboard, side rails.

Cleaning and disinfection after a patient leaving or before a transfer:

- Headboard, footboard, side rails, crib base, brake, bumpers, IV Pole, fairings.

Exhaustive cleaning and disinfection each two months:

- The entire crib.

MAINTENANCE

Always check the correct state of:


- Trendelenburg / Reverse Trendelenburg mechanism.
- Side rails mechanism.
- Wheels.
- Braking system.

For more information, please consult the use and maintenance manual.



INSTRUCTIONS OF USE

A	Raising crib	B	Lowering crib
---	--------------	---	---------------

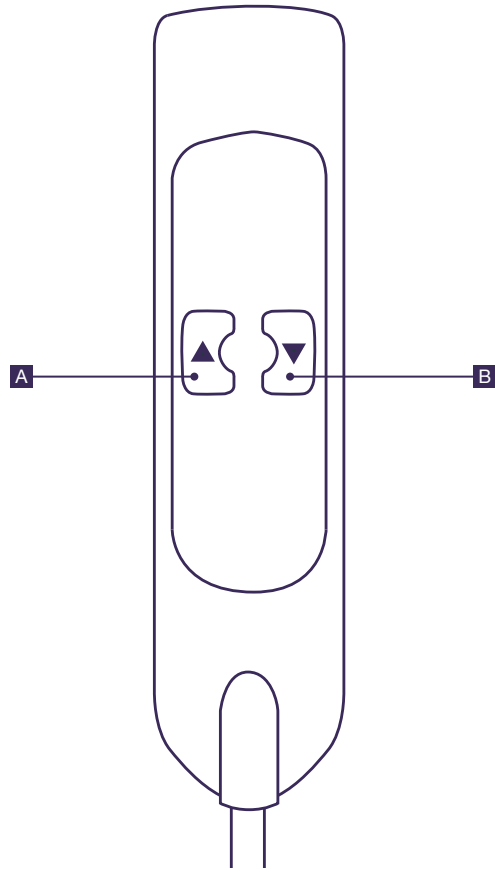

Control for raising / lowering of the crib

Industrias Hidráulicas Pardo S.L. company has the following certifications:



SAFETY WARNINGS

- Before raising and lowering the moving parts of the module, with the other parts of the crib or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- The crib should be in its horizontal position when the patient is not being cared for, in order to reduce the risk of injury from falling.

